

An efficient transport back-transport framework for EIT

Alexandre Fouchard^{1,2}, S. Bonnet¹, L. Hervé¹ and Olivier David²

¹CEA, Leti, 17 rue des Martyrs, 38000 GRENOBLE, France, alexandre.fouchard@centraliens-lyon.net

²Univesité Joseph Fourier, Grenoble Institute of Neuroscience, Bât. E.J. Safra, Chemin Fortuné Ferrini, 38700 La Tronche, France

Abstract: Implementation of efficient methods to handle calculations in EIT is a key issue to address 3D electrical property reconstructions. Following a transport back-transport method, we develop in this work an adjoint approach and define explicit forward and back-projection operators. It allows reducing the size of matrices involved in reconstruction. This framework has been tested on experimental data acquired *in vitro* on a saline phantom.

1 Introduction

Forward problem solution and sensitivity computations are the fundamentals of Electrical Impedance Tomography (EIT) [1]. Standard approach is to use Finite Element Methods (FEM) to derive both admittance matrix and Jacobian from an elemental discretization of conductivity. Calculation parallelization [2] and deduction of nodal Jacobian [3] offer ways to enhance calculus efficiency.

In most EIT systems, the same measurement configuration is used per injection configuration. Then, following a transport back-transport method [4], we explicitly define forward and back-projection operators from potential gradients. It allows using inversion algorithms without explicit Jacobian assembly. Matrix size involved in reconstruction is proportional to the number of electrodes E instead of the number of measurements.

2 Methods

We elaborate our framework supposing the electric potential $\mathbf{v} \in \mathbb{R}^{N_n}$ linear per element and considering a piecewise constant conductivity discretization $\boldsymbol{\sigma} \in \mathbb{R}^{N_e}$.

2.1 Sensitivity calculations, adjoint framework

Classical estimation of Jacobian coefficient is based on the perturbation approach [5]. Two configurations are considered: the actual measurement configuration, and a virtual measurement configuration in which source and detector have been interchanged. In this work, the Jacobian matrix is factorized with matrices containing elemental potential gradients. They can be determined by standard FEM formulation [6]. Using only the gradient matrices, a forward operator is defined and solves a direct transport problem. A back-projection operator is also defined and transports back residuals into the imaging domain. The profit of such a formulation relies upon the size of gradient matrices $\mathbf{G} \in \mathbb{R}^{N_e \times E}$ used in inversion, versus the larger size of standard Jacobian matrix, typically $\mathbf{J} \in \mathbb{R}^{N_e \times E^2}$. Inversion is then done with a standard preconditioned conjugate gradient (PCG).

2.2 Experimental device

Experimental measurements are performed on a saline phantom of 4cm diameter featuring 14 equally-spaced copper electrodes with a custom-built EIT system [7].

2.2.1 Reconstruction approach

The implementation of the framework, adapted from the EIDORS library [8], is first validated on simple test cases in 2D before exploring reconstructions from noisy simulated measurements. Reconstructions are then performed against experimental data.

3 Results

Reconstructions from simulated data (Figure 1) exhibit a correct behaviour of the framework and PCG algorithm used for inversion. The framework performs also well in experimental situation (Figure 2).

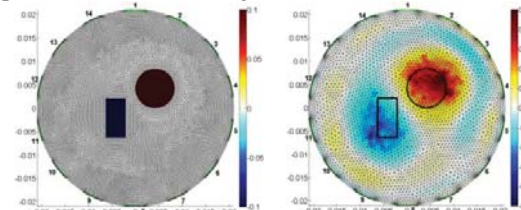


Figure 1: 2D difference reconstructions from simulated data with 5% additive Gaussian noise

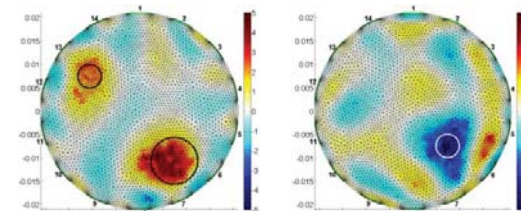


Figure 2: 2D difference reconstruction from experimental data, with estimated 5% noise

4 Discussion

The framework presented in this work allows inversion without explicit Jacobian calculations, working only with potential gradient matrices for injection and measurement configuration. It has been validated against both simulated and *in vitro* experimental measurements.

Further investigation might consider reconstructions that favour sparse solutions and make use of non-linear inversion algorithms.

References

- [1] Lionheart W R B, *Physiol Meas*, **25**(1):125, 2004
- [2] Borsic A, Attardo E A, Halter R J, *Physiol Meas*, **33**(10):1703, 2012
- [3] Graham B M, Adler A, *Int J Inf Syst Sci*, **2**:453–68, 2006
- [4] Dom O, *Inverse Problems*, **14**:1107-30, 1998
- [5] Geselowitz D B, *IEEE Trans Biomed Eng*, **18**(1):38–41, 1971
- [6] Vavasis S A, *SIAM J. Numer. Anal.*, **33**(3):890-916, 1996
- [7] Fouchard A, Noca A, Bonnet S, Pham P, Clarençon D, David O, submitted in *IEEE EMBC*, 2014
- [8] Adler A, Lionheart W R B, *Physiol Meas*, **27**:S25-42, 2006

Excerpted from:

Proceedings
of the
15th International Conference on
Biomedical Applications of
**ELECTRICAL IMPEDANCE
TOMOGRAPHY**

Edited by Andy Adler and Bartłomiej Grychtol

April 24-26, 2014
Glen House Resort
Gananoque, Ontario
Canada



This document is the collection of papers accepted for presentation at the 15th International Conference on
Biomedical Applications of Electrical Impedance Tomography.
Each individual paper in this collection: © 2014 by the indicated authors.
Collected work: © 2014 Andy Adler and Bartłomiej Grychtol.
All rights reserved.

Cover design: Bartłomiej Grychtol
Photo credit: ©1000 Islands Photo Art Inc. / Ian Coristine

Printed in Canada

ISBN 978-0-7709-0577-4

Systems and Computer Engineering
Carleton University, 1125 Colonel By Drive
Ottawa, Ontario, K1S 5B6, Canada
adler@sce.carleton.ca
+1 (613) 520-2600

www.eit2014.org