

3-D Electrical Impedance Tomography Reconstruction Using ℓ_1 Norms Regularization

Yang Pu, Qifan Wang and Tao Dai

Sealand Technology (Chengdu), Ltd., Chengdu, China. ypu@eitchina.net

Abstract: An ℓ_1 norm reconstruction algorithm which has the merits of reducing the sensitivity to data outliers and avoiding edge blurring is applied in this paper to solve a 3-D EIT problem. The iterative imaging method allows flexible choice of norms by simply choosing different norm value. A cluster analysis is implemented for labelling targets using the morphology technique.

1 Introduction

Electrical Impedance Tomography (EIT) is a soft field imaging modality due to the diffusive propagation of electrical current. Reconstruction of the internal conductivity distribution from boundary measurements is severely ill-conditioned. Most reconstruction algorithms are based on ℓ_2 norm regularization (e.g. one-step GN method) which is believed to blur image outlines and be sensitive to measurement noises. These difficulties can be greatly alleviated if ℓ_1 norm reconstruction technique is involved [1-5]. An ℓ_1 norm applied on the measurements residue term reduces the sensitivity to data outliers, while an ℓ_1 norm on the image prior term avoids edge blurring. An ℓ_1 norm iterative method is applied in this paper to solve a 3-D EIT problem, which is designed to detect breast cancer from women patients. In the post-processing stage, a cluster analysis is applied for labelling reconstructed targets using the morphology technique. Simulative and phantom experiments showed the advantages of ℓ_1 norm reconstruction and the validity of the clustering method.

2 Methods

A weighted and regularized inverse seeks an estimate solution $\hat{\mathbf{x}}$ by minimizing

$$\hat{\mathbf{x}} = \underset{\mathbf{x}}{\operatorname{argmin}} \|\mathbf{y} - \mathbf{J}\mathbf{x}\|_{\Sigma_n}^{p_n} + \|\mathbf{x} - \mathbf{x}^0\|_{\Sigma_x}^{p_x} \quad (1)$$

Where p_n and p_x are the data and image norms respectively. With $p_n = 2$, $p_x = 2$ it models the ℓ_2 norm regularization; while with $p_n = 1$, $p_x = 1$, ℓ_1 norm reconstruction can be achieved. In this paper, a general iterative method for solving (1) is applied, which allows flexible choice of norms by simply choosing different p_n and p_x value. Details can be found in [5], and will not be elaborated here.

When EIT reconstruction is completed, image filtering technique is implemented to remove noises, and then a cluster analysis based on the morphology is involved for labelling targets.

3 Results

3.1 Numerical simulation

The forward model was a funnel-shaped applicator. 64 electrodes were located surrounding the outside surface.

Inside, there were two targets with conductivity $1.2 \times \sigma_h$, while the background had conductivity $\sigma_h = 1$. In order to accurately simulate forward model and make inverse solution less ill-conditioned, dual model was applied, which means a fine mesh for the forward and coarse mesh for the inverse. Gaussian white noise was added to the simulation data with noise level SNR=20dB. When reconstruction was completed, cluster analysis was implemented. The two targets were marked by different colours (red and yellow) as shown in Fig. 1.

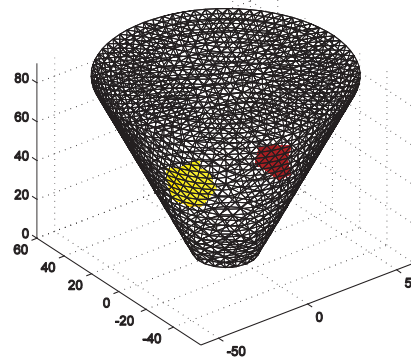


Figure 1: Image reconstructed using ℓ_1 norm and labelled by cluster analysis.

3.2 Phantom experiment

The saline phantom was fabricated the same as described in the previous section. Small biological tissues such as potato, apple and porcine liver were statically suspended in the saline solution. Similar results were obtained.

4 Conclusions

EIT images reconstructed using ℓ_1 norm regularization give two distinct advantages: edge preservation and noise robustness. However, the disadvantage is that the ℓ_1 norm formulation cannot be realized as a linear one-step algorithm due to non-differentiability. In this paper, we extended Dai's previous work [5] from 2-D to 3-D problem, and proved that the iterative process for solving (1) is effective in 3-D scenario as well. Moreover, the cluster analysis based on the morphology technique was involved and successfully separated targets from the background, which is important in clinical applications.

References

- [1] Y. Mamatjan, *Physiol Meas*, 34:1027–1039, 2013
- [2] Y. Mamatjan, Canadian Medical and Biological Engineering Society (CMBEC 35) and Canada Clinical Engineering Society (ACCES 17) conference, June 19–22, Halifax, Canada, 2012
- [3] A. Borsic, *Inverse Problems*, 28:095011, 2012
- [4] A. Borsic, *IEEE Trans. Medical Imaging*, 29: 44–54, 2010
- [5] T. Dai, *Conf. IEEE Eng. Med. Biol. Soc.*, Vancouver, Canada, August 20–24, 2008

Excerpted from:

Proceedings
of the
15th International Conference on
Biomedical Applications of
**ELECTRICAL IMPEDANCE
TOMOGRAPHY**

Edited by Andy Adler and Bartłomiej Grychtol

April 24-26, 2014
Glen House Resort
Gananoque, Ontario
Canada



This document is the collection of papers accepted for presentation at the 15th International Conference on
Biomedical Applications of Electrical Impedance Tomography.
Each individual paper in this collection: © 2014 by the indicated authors.
Collected work: © 2014 Andy Adler and Bartłomiej Grychtol.
All rights reserved.

Cover design: Bartłomiej Grychtol
Photo credit: ©1000 Islands Photo Art Inc. / Ian Coristine

Printed in Canada

ISBN 978-0-7709-0577-4

Systems and Computer Engineering
Carleton University, 1125 Colonel By Drive
Ottawa, Ontario, K1S 5B6, Canada
adler@sce.carleton.ca
+1 (613) 520-2600

www.eit2014.org